


Physician:
Patient: **Sample Report**
Accession #:
Sex: F Age: 56
Date of Birth:
Collected:

IgA
IgG
IgE


CLIA #: 50D0965661
© US BioTek Laboratories

Dairy


Bovine-derived unless specified

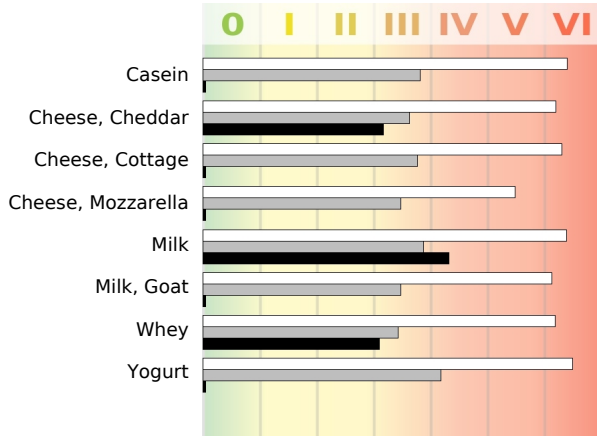


Fruits

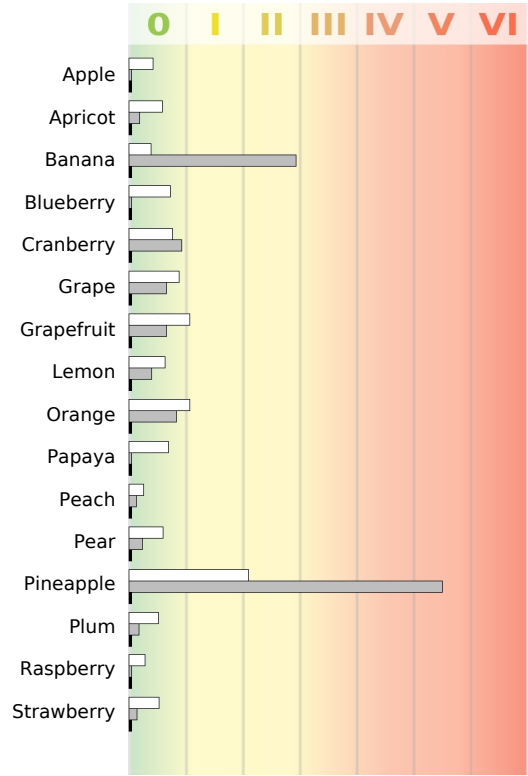


Meat/Fowl

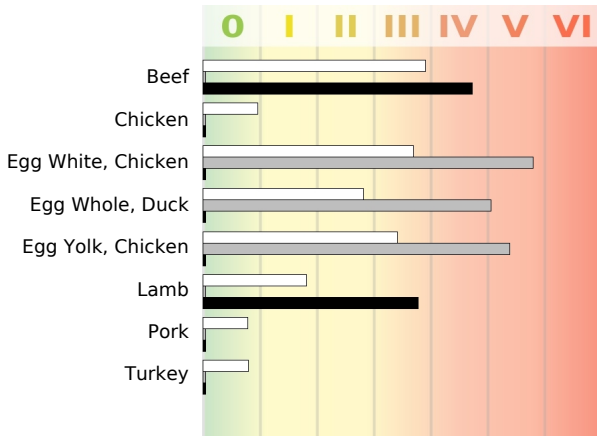

Fish/Crustacea/Mollusk

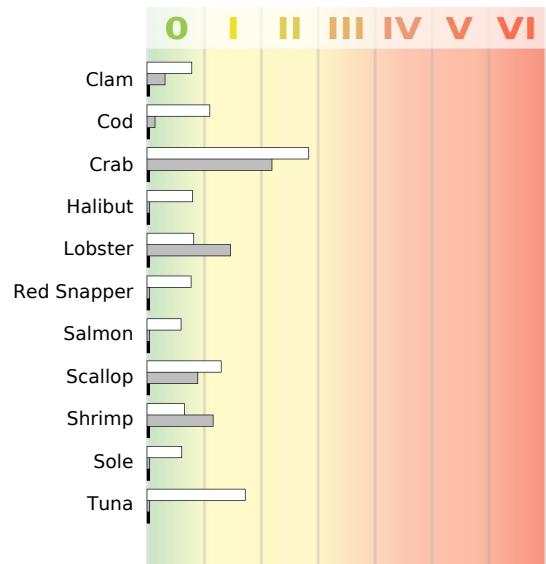

Misc

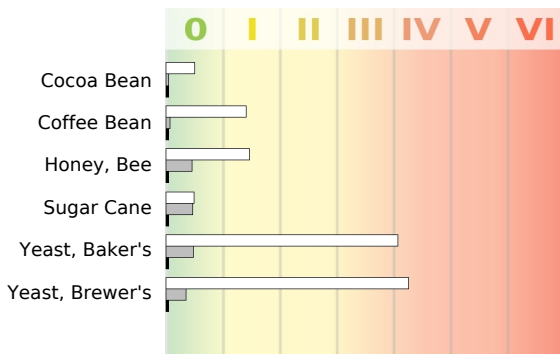

Reaction Class




This test does not identify anaphylaxis. Low allergen-IgE cannot justify secondary exposure to food suspect of inducing anaphylaxis as it may prove fatal. This test is not intended to diagnose, treat, cure, or prevent any disease or replace the medical advice and/or treatment obtained from a qualified healthcare practitioner. US BioTek's proprietary ELISA analysis is a semi-quantitative assessment for specific Total IgG (subclasses 1, 2, 3, 4) and IgE antibodies. The classification of 0 to VI denotes the level of IgG, IgA, and/or IgE antibodies detected through spectrophotometric analysis. US BioTek Laboratories, Inc. has developed and determined the performance characteristics of this test under the Clinical Laboratory Improvement Amendments (CLIA). This test has not been evaluated by the U.S. Food and Drug Administration and is considered for investigational and research purposes only. IgG and IgA antibodies may be associated with Delayed-Onset Hypersensitivity Reactions. IgE antibodies may be associated with Immediate-Onset Hypersensitivity Reactions. The antigens on the panel are subject to change without prior notice. Reference ranges are updated periodically.

Physician:
 Patient: **Sample Report**
 Accession #:
 Sex: F Age: 56
 Date of Birth:
 Collected: Received: Completed:


IgA
 IgG
 IgE

CLIA #: 50D0965661
 © US BioTek Laboratories

Grains/Legumes/Nuts

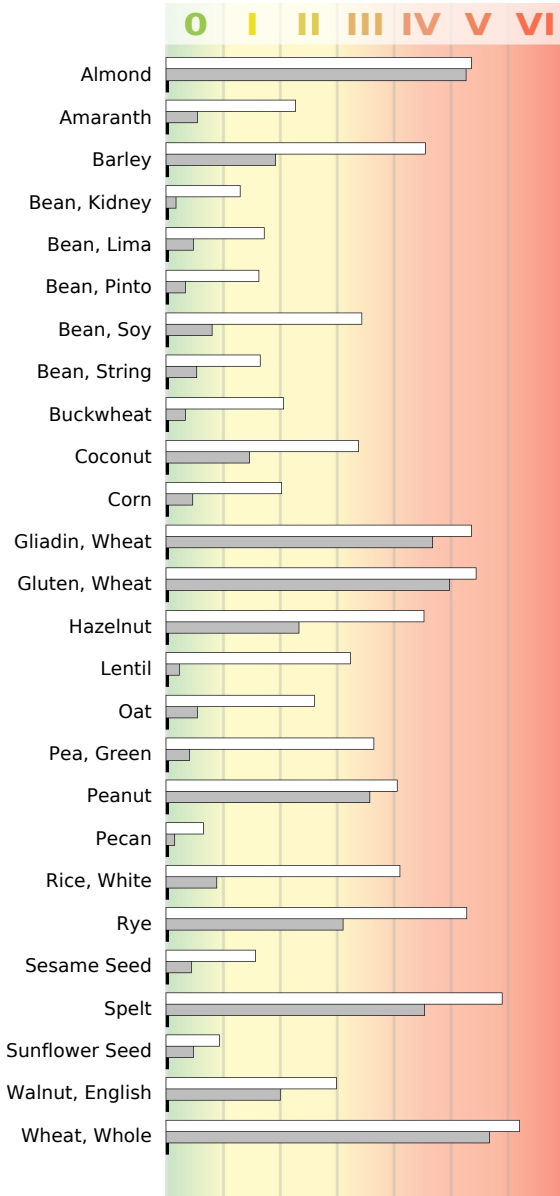

Vegetables

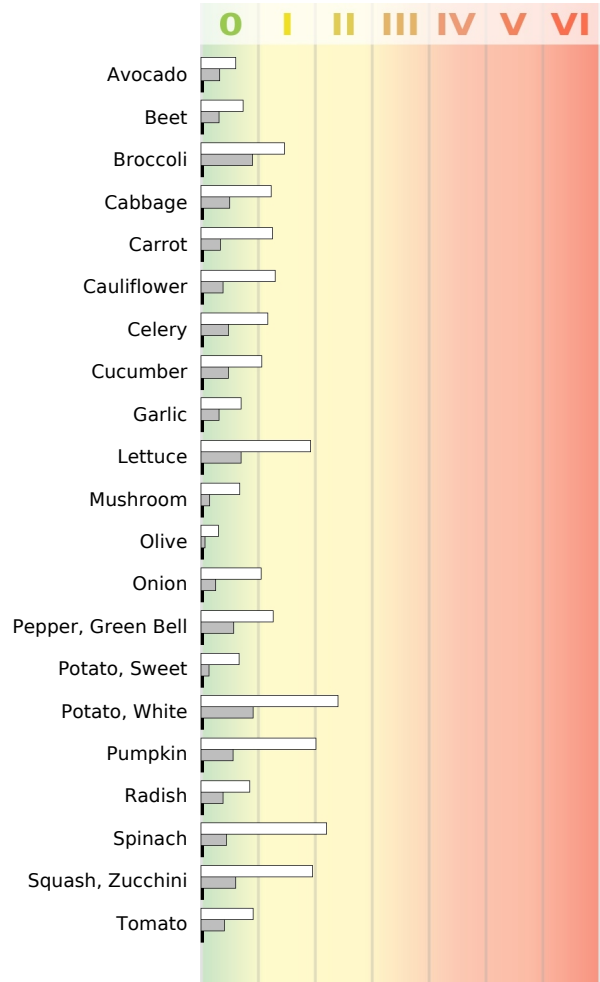

Reaction Class



This test does not identify anaphylaxis. Low allergen-IgE cannot justify secondary exposure to food suspect of inducing anaphylaxis as it may prove fatal. This test is not intended to diagnose, treat, cure, or prevent any disease or replace the medical advice and/or treatment obtained from a qualified healthcare practitioner. US BioTek's proprietary ELISA analysis is a semi-quantitative assessment for specific Total IgG (subclasses 1, 2, 3, 4) and IgE antibodies. The classification of 0 to VI denotes the level of IgG, IgA, and/or IgE antibodies detected through spectrophotometric analysis. US BioTek Laboratories, Inc. has developed and determined the performance characteristics of this test under the Clinical Laboratory Improvement Amendments (CLIA). This test has not been evaluated by the U.S. Food and Drug Administration and is considered for investigational and research purposes only. IgG and IgA antibodies may be associated with Delayed-Onset Hypersensitivity Reactions. IgE antibodies may be associated with Immediate-Onset Hypersensitivity Reactions. The antigens on the panel are subject to change without prior notice. Reference ranges are updated periodically.